

Allweighs Weighing Services
 Westend Grange
 West End Road
 Epworth
 Doncaster
 DN9 1LA
 Tel: 01427 875 867
 Web: www.allweighs.co.uk



Certificate No: CJS:

2023000507

Location: Factory

Manufacturer: Locosc LP7510B

Serial/Plant No: 20170722020

Capacity: 3000 kg

Increment: 1 kg

Frequency: 12 months

Test Date: 14 December 2023

Next due: December 2024

Calibration Certificate of Accuracy

Business Name: Advanced Metal Innovation Co.

Address: Wagon Works
 Rotherham Road
 Sheffield
 S20 1AH

Contact Name: Jay

Off-centre Loading:

Load point:	Reading:	Deviation:	Load point:	Reading:	Deviation:
1	10660	0			
2	10660	0			
3	10660	0			
4	10660	0			

Four loadcell Six loadcell

Single loadcell Eight loadcell

As Found

Measurement Points:	Reading:	Deviation:
0	0	0
400	400	0
800	800	0
1000	1000	0
2000	2000	0
3000	3000	0

Repeatability

2000	2000	0
------	------	---

Definitive

Measurement Points:	Reading:	Deviation:
0	0	0
400	400	0
800	800	0
1000	1000	0
2000	2000	0
3000	3000	0

Repeatability

2000	3000	0
------	------	---

Notes:

Engineer Name:

CJS

C. Scott

Traceable Weights Used:

W23003

Trading Standards Maximum Tolerance:

3


+/-

3

kg

Calibration method and equipment used traceable to national standards.

QMF17 Issue 5 14/07/2020



Allweighs Weighing Services
 Westend Grange
 West End Road
 Epworth
 Doncaster
 DN9 1LA
 Tel: 01427 875 867
 Web: www.allweighs.co.uk



Certificate No: CJS:

2023000506

Location: Weighbridge

Manufacturer: DINI Argeo 3590ET

Serial/Plant No: 83626662

Capacity: 50000 kg

Increment: 20 kg

Frequency: 12 months

Test Date: 14 December 2023

Next due: December 2024

Calibration Certificate of Accuracy


Business Name: Advanced Metal Innovation Co.

Address: Wagon Works
 Rotherham Road
 Sheffield
 S20 1AH

Contact Name: Jay

Off-centre Loading:

Load point:	Reading:	Deviation:	Load point:	Reading:	Deviation:
1	10660	0	5	10660	0
2	10660	0	6	10660	0
3	10660	0			
4	10660	0			

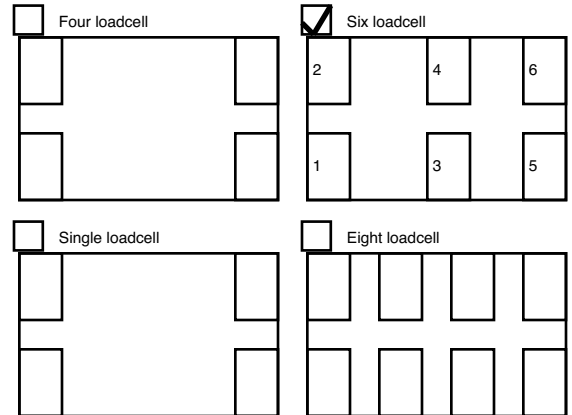

As Found

Measurement Points:	Reading:	Deviation:
0	0	0
8000	8000	0
16000	16000	0
23660	23660	0
33660	33660	0
43840	43840	0

Repeatability

43840	43840	0
-------	-------	---

Notes:

Engineer Name:

CJS

C. Scott

Definitive

Measurement Points:	Reading:	Deviation:
0	0	0
8000	8000	0
16000	16000	0
23660	23660	0
33660	33660	0
43840	43840	0

Repeatability

43840	43840	0
-------	-------	---

Traceable Weights Used: W23003

Trading Standards Maximum Tolerance: 60 +/- 60 kg

Calibration method and equipment used traceable to national standards.

QMF17 Issue 5 14/07/2020